William Laboratories, Inc.

Safe-T-Vue® 10 • Product No. 7201

QUALITY ASSURANCE LOT PERFORMANCE REPORT

Safe-T-Vue® 10 Non-Reversible Temperature Indicator Product No. 7201

PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 10 IS PRINTED IN BLACK.

Lot # S10 110613

Expiration Date: 2015-11

Non - Chemistry

Mark √ for "Accepted" and X for "Not Accepted."

Box	Adh. Label	Foil Lid	Close Function	Fill Level
√ Copy	√ Copy	√ Copy	√ Formed	√ Acceptable
√ Tack	√ Tack	√ Position	√ Locked/Stable	Underfill
√ Clean	√ Color	√ Clean Peel	**Hinge**	Overfill
√ Box Damage	**Tray**	**Disk**	√ Elasticity	**Color Label**
	√ Edges	√ Appearance		√ Color
	√ Color	√ Fit		

Test Protocol – Finished Goods Quality Assurance

Test performed on random sampling of finished product per ANSI ASQZ1.4-2003

Data from a "DigiSense" Thermister Electronic Thermometer, using a cold (start temperature 1° to 5° C) bag of simulated blood (10% glycerol-water) with thermometer probe positioned in center of blood bag. Agitation of blood bag necessary for collection of accurate temperature-color change data. Download detailed protocol, from www.williamlabs.com, QCP/0200-5," Receiving Inspection – Temperature Indicators". [Important: 7206 has a specific incoming inspection protocol.]

Temperature Change and Corresponding Safe-T-Vue® Change

Sample Set 1	DATA	Sample Set 2
1 to 5 °C	*Starting Temperatures*	1 to 5 °C

OBSERVATIONS

Temperature		Color Change	
9.2	°C	Red Spots - Random	WHITE CENTER
9.7	°C	Red Filling In	WHITE CENTER
10.0	°C	Full Red Color	RED CENTER

Temperature		Color Change	
9.2	°C	Red Spots - Random	WHITE CENTER
9.7	°C	Red Filling In	WHITE CENTER
10.0	°C	Full Red Color	RED CENTER

Temperature accuracy is +/-0.3°C.

Results: Red Spots - Random 9.2 ° C; Red Filling in White Center 9.7 ° C; Full Red Color at 10.0 ° C.

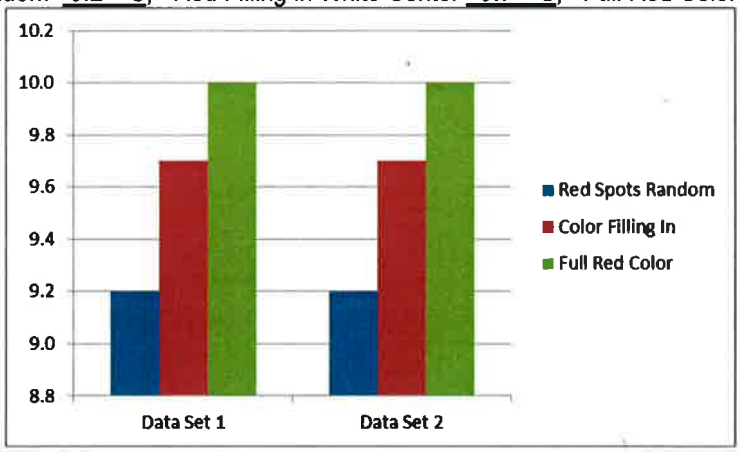

QUALITY ASSURANCE: APPROVED LOT # S10 110613 ;

QAP/0102-2, REV 08, November 24, 2009

Sr QE Manager

31DEC13

Date