

**Safe-T-Vue® 6 • Product No. 7206**

**QUALITY ASSURANCE LOT PERFORMANCE REPORT**

Safe-T-Vue® 6 Non-Reversible Temperature Indicator Product No. 7206

PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 6 IS PRINTED IN BLACK.

Lot # **S6 090313**

Expiration Date: 2015-09

**Non - Chemistry**

Mark  $\checkmark$  for "Accepted" and X for "Not Accepted."

Box	Adh. Label	Foil Lid	Close Function	Fill Level
$\checkmark$ Copy	$\checkmark$ Copy	$\checkmark$ Copy	$\checkmark$ Formed	$\checkmark$ Acceptable
$\checkmark$ Tack	$\checkmark$ Tack	$\checkmark$ Position	$\checkmark$ Locked/Stable	Underfill
$\checkmark$ Clean	$\checkmark$ Color	$\checkmark$ Clean Peel	<b>Hinge</b>	Overfill
$\checkmark$ Box Damage	<b>Tray</b>	<b>Disk</b>	$\checkmark$ Elasticity	<b>Color Label</b>
	$\checkmark$ Edges	$\checkmark$ Appearance		$\checkmark$ Color
	$\checkmark$ Color	$\checkmark$ Fit		

**Test Protocol – Finished Goods Quality Assurance**

*Test performed on random sampling of finished product per ANSI ASQZ1.4-2003*

Data from a "DigiSense" Thermister Electronic Thermometer, using a cold (start temperature 1° to 5° C) bag of simulated blood (10% glycerol-water) with thermometer probe positioned in center of blood bag. Agitation of blood bag necessary for collection of accurate temperature-color change data. Download detailed protocol, from [www.williamlabs.com](http://www.williamlabs.com), QCP/0200-5, "Receiving Inspection – Temperature Indicators". [Important: 7206 has a specific incoming inspection protocol.]

**Temperature Change and Corresponding Safe-T-Vue® Change**

Sample Set 1	DATA	Sample Set 2
1 to 2 °C	Starting Temperatures	1 to 2 °C


**OBSERVATIONS**

Temperature	Color Change
4.0 °C	Red Spots - Random WHITE CENTER
5.4 °C	Red Filling In WHITE CENTER
6.0 °C	Full Red Color RED CENTER

Temperature	Color Change
3.8 °C	Red Spots - Random WHITE CENTER
5.3 °C	Red Filling In WHITE CENTER
6.0 °C	Full Red Color RED CENTER

Temperature accuracy is +/-0.3°C.

**Results:** Red Spots - Random 3.9 °C; Red Filling in White Center 5.4 °C; Full Red Color at 6.0 °C.

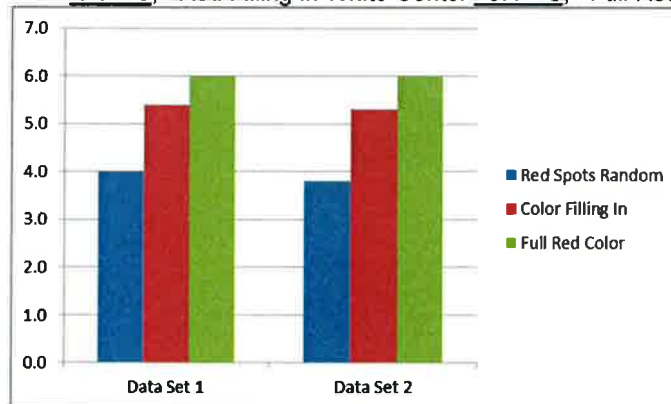

**QUALITY ASSURANCE: APPROVED LOT # S6 090313 ;**

QAP/0102-2, REV 08, November 24, 2009

*M. S. Mahager*  
Sr QE Mahager

09 JAN 14  
Date